

QUICK INSTALLATION GUIDE


Installation Instructions



The DCI 3 Position Deluxe Power Pack is preset to operate like any standard power optics light source system. The preset output voltage is 3.3 VDC (Setting #5) and the system is programmed to provide light when the foot control is activated. Program setting #9.

For a new installation:

1. Turn the dental unit OFF and disconnect power.
2. Install a 1/8" X 1/8" X 1/16" tee fitting in the drive air line on the desired handpiece tubing.
3. Attach 1/8" tubing from the tee fitting to the proper handpiece position air signal input on the power optics source.
4. Install light source wiring to power pack.
5. Complete steps 2 & 3 with the remaining handpiece positions as necessary.
6. Set the voltage setting knob to 0 for unused handpiece positions.
7. Attach input power wires to the power optics source.
8. Turn the dental unit on and verify your new installation operates properly. Ensure a handpiece is installed to create back pressure to operate the power optics source.

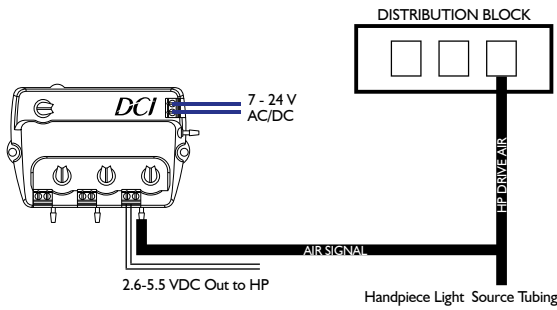

FOR ADVANCED PROGRAM SETTINGS AND INSTALLATION OPTIONS
REFER TO THE USER INSTALLATION MANUAL 92518

PN 92681, Rev. A, 3/16

www.dcionline.com
800-624-2793

305 N. Springbrook Road
Newberg, OR 97132, USA

QUICK INSTALLATION GUIDE


Installation Instructions



The DCI 3 Position Deluxe Power Pack is preset to operate like any standard power optics light source system. The preset output voltage is 3.3 VDC (Setting #5) and the system is programmed to provide light when the foot control is activated. Program setting #9.

For a new installation:

1. Turn the dental unit OFF and disconnect power.
2. Install a 1/8" X 1/8" X 1/16" tee fitting in the drive air line on the desired handpiece tubing.
3. Attach 1/8" tubing from the tee fitting to the proper handpiece position air signal input on the power optics source.
4. Install light source wiring to power pack.
5. Complete steps 2 & 3 with the remaining handpiece positions as necessary.
6. Set the voltage setting knob to 0 for unused handpiece positions.
7. Attach input power wires to the power optics source.
8. Turn the dental unit on and verify your new installation operates properly. Ensure a handpiece is installed to create back pressure to operate the power optics source.

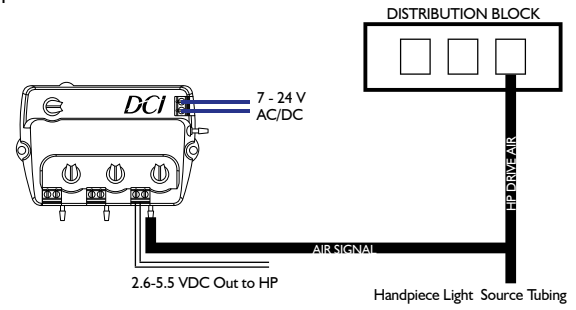

FOR ADVANCED PROGRAM SETTINGS AND INSTALLATION OPTIONS
REFER TO THE USER INSTALLATION MANUAL 92518

PN 92681, Rev. A, 3/16

www.dcionline.com
800-624-2793

305 N. Springbrook Road
Newberg, OR 97132, USA

QUICK INSTALLATION GUIDE


Installation Instructions



The DCI 3 Position Deluxe Power Pack is preset to operate like any standard power optics light source system. The preset output voltage is 3.3 VDC (Setting #5) and the system is programmed to provide light when the foot control is activated. Program setting #9.

For a new installation:

1. Turn the dental unit OFF and disconnect power.
2. Install a 1/8" X 1/8" X 1/16" tee fitting in the drive air line on the desired handpiece tubing.
3. Attach 1/8" tubing from the tee fitting to the proper handpiece position air signal input on the power optics source.
4. Install light source wiring to power pack.
5. Complete steps 2 & 3 with the remaining handpiece positions as necessary.
6. Set the voltage setting knob to 0 for unused handpiece positions.
7. Attach input power wires to the power optics source.
8. Turn the dental unit on and verify your new installation operates properly. Ensure a handpiece is installed to create back pressure to operate the power optics source.

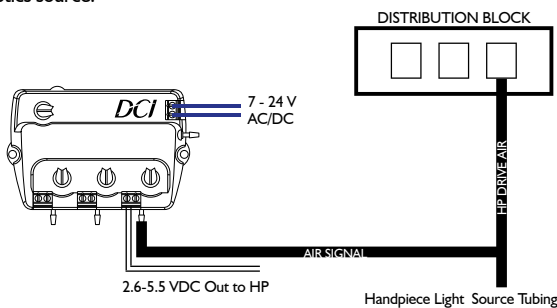

FOR ADVANCED PROGRAM SETTINGS AND INSTALLATION OPTIONS
REFER TO THE USER INSTALLATION MANUAL 92518

PN 92681, Rev. A, 3/16

www.dcionline.com
800-624-2793

305 N. Springbrook Road
Newberg, OR 97132, USA

QUICK INSTALLATION GUIDE


Installation Instructions



The DCI 3 Position Deluxe Power Pack is preset to operate like any standard power optics light source system. The preset output voltage is 3.3 VDC (Setting #5) and the system is programmed to provide light when the foot control is activated. Program setting #9.

For a new installation:

1. Turn the dental unit OFF and disconnect power.
2. Install a 1/8" X 1/8" X 1/16" tee fitting in the drive air line on the desired handpiece tubing.
3. Attach 1/8" tubing from the tee fitting to the proper handpiece position air signal input on the power optics source.
4. Install light source wiring to power pack.
5. Complete steps 2 & 3 with the remaining handpiece positions as necessary.
6. Set the voltage setting knob to 0 for unused handpiece positions.
7. Attach input power wires to the power optics source.
8. Turn the dental unit on and verify your new installation operates properly. Ensure a handpiece is installed to create back pressure to operate the power optics source.

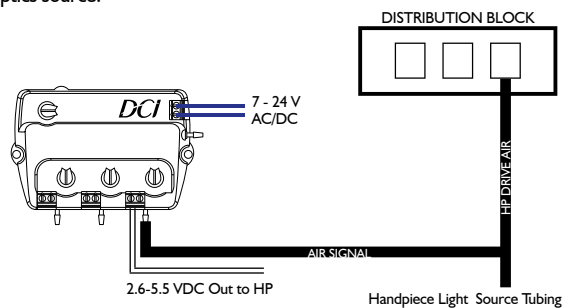

FOR ADVANCED PROGRAM SETTINGS AND INSTALLATION OPTIONS
REFER TO THE USER INSTALLATION MANUAL 92518

PN 92681, Rev. A, 3/16

www.dcionline.com
800-624-2793

305 N. Springbrook Road
Newberg, OR 97132, USA